

PAPER • OPEN ACCESS

Pulse Shape Discrimination with EJ299 scintillators

To cite this article: A Muoio *et al* 2018 *J. Phys.: Conf. Ser.* **966** 012064

View the [article online](#) for updates and enhancements.

You may also like

- [Optimization of fast neutron and X-ray pulse shape discrimination \(PSD\) using an EJ276G scintillator in high radiation mixed conditions](#)
G. Song, S. Lee, J. Park et al.
- [Hybrid additive manufacturing of 3D electronic systems](#)
J Li, T Wasley, T T Nguyen et al.
- [Comparative study of large samples \(2" x 2"\) plastic scintillators and EJ309 liquid with pulse shape discrimination \(PSD\) capabilities](#)
J Iwanowska-Hanke, M Moszynski, L Swiderski et al.



The Electrochemical Society
Advancing solid state & electrochemical science & technology

247th ECS Meeting
Montréal, Canada
May 18-22, 2025
Palais des Congrès de Montréal

Showcase your science!

Abstract submission deadline extended: December 20

ECS UNITED

The poster features a large graphic of a hand holding a globe with three vertical bars, set against a background of a grid of dots and wavy lines. The ECS logo is in the top left, and the meeting details are in the top right. A green circle in the bottom right contains the text about the extended abstract submission deadline.

Pulse Shape Discrimination with EJ299 scintillators

A Muoio^{1,2}, F Cappuzzello^{1,2}, D Carbone¹, M Cavallaro¹, G Lanzalone^{1,3}, A Pappalardo⁴, G Santagati¹, A Trifirò^{5,6}, S Tudisco¹

¹INFN - LNS, Via S. Sofia 62, 95123 Catania, Italy

²Dip. di Fisica e Astronomia, Univ. di Catania, Via S. Sofia 64, 95123 Catania Italy

³Univ. Degli Studi di Enna “Kore”, Via delle Olimpiadi, 94100 Enna, Italy

⁴ELI-NP (Extreme Light Infrastructure-Nuclear Physics, Magurele, Romanian

⁵Dip. di Scienze MIFT, Univ. degli Studi di Messina, Viale F.S. D’Alcontres 31, 98166 Messina, Italy

⁶INFN - Sez. di Catania, Via S. Sofia 64, 95123 Catania, Italy

Abstract. Recently a new generation plastic scintillator PPO have been developed. They promise excellent performances in terms of neutron/gamma discrimination. In this work we will present the activity made at INFN-LNS on the plastic scintillator EJ299 in comparison with the most traditional liquid scintillator EJ301 used in several nuclear physics experiments.

In the past scintillation detectors have been used in several nuclear physics studies [1-3] and applications [4,5]. Recently, the possibility of manufacturing plastic scintillators with efficient neutron/gamma discrimination has been developed with a new polyvinyltoluene (PVT) polymer matrix loaded with a scintillating dye, 2,5-diphenyloxazole (PPO) [6].

Recently at INFN-LNS two research topics are fostering R&D on these scintillators, the study of Double Charge Exchange (DCE) in peripheral nuclear reactions[7] and Nuclear Reactions and astrophysics process in Plasmas (NRP) [8].

The exploration of detailed nuclear structure through DCE has historically got great benefits by the use of magnetic spectrometers. Recently large acceptance and high resolution spectrometers have been installed in leading European laboratories for fundamental nuclear physics with a major impact on the progress of knowledge in several branches of nuclear structure and reaction mechanisms.

Important upgrading of the existing facilities can be foreseen, especially in the view of emerging detection technologies, in order to extend the application of magnetic spectrometry to the more and more challenging experiments required by the present and future nuclear science. Among these, the MAGNEX spectrometer [9] of LNS has been coupled to organic scintillators neutron detector array, EDEN [10,11], to perform a better selection of reaction mechanisms. The improvement of PPO technology could be very useful to these topics.

NRP is a new field of studies related to recent laser technology advances, which in the near future can give the opportunity to investigate nuclear reactions and fundamental process in plasma under extreme conditions. Also for this contest, the “ideal” neutron detection module must have: i) high efficiency; ii) good discrimination of gammas from neutrons; iii) good timing performance for ToF neutron energies reconstruction.



In addition, laser-plasma experiments require detector able to work in hard environmental conditions. These requirements may be met by configuration based on plastic scintillators coupled with new solid state devices, Silicon Photomultiplier, SiPM [12][13][14], and a totally digital acquisition for the multi-hit signals expected from reactions events in plasma. In this work we found that the response of liquid scintillator is characterized by rise times of the order of 3-4 ns. One advantage of plastic scintillators include fairly high light output, with a rise time of 2-4 nanoseconds, but one of the major advantages is their flexibility. They are easily machined by normal means and shaped to desired forms. A special focus on the pulse shape discrimination capability of this material, which is characterized by low toxicity and low volatility, has been addressed. A possibility of manufacturing plastic scintillators with efficient neutron/gamma pulse shape discrimination is demonstrated using a system of a PVT polymer matrix loaded with a PPO. According to a commonly accepted mechanism [15] [16], both gamma and neutron induced pulses contain a fast decay (prompt) component and a slow decay (delayed) fluorescence one.

In order to characterize Pulse Shape Discrimination (PSD) for the two detectors the following experimental set-up was done.

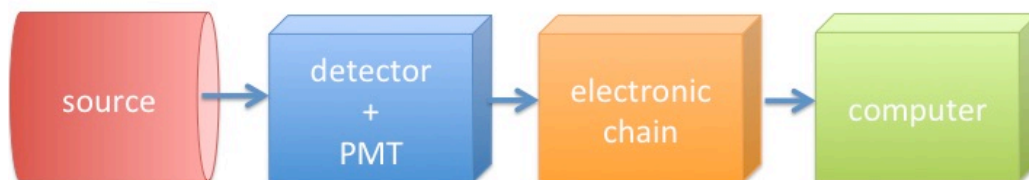


Figure 1 A sketch of experimental setup.

The first test on detectors was performed on liquid scintillator EJ301 + PMT (Photo Multiplier Tube) Hamamatsu R 1250. The liquid scintillator has been assembled and oriented towards the Am-Be source collimated through an aluminium plate 2 cm thick with a hole of 5 mm diameter, in order to keep less than 5% the difference in the path length of particles impinging in the detectors.

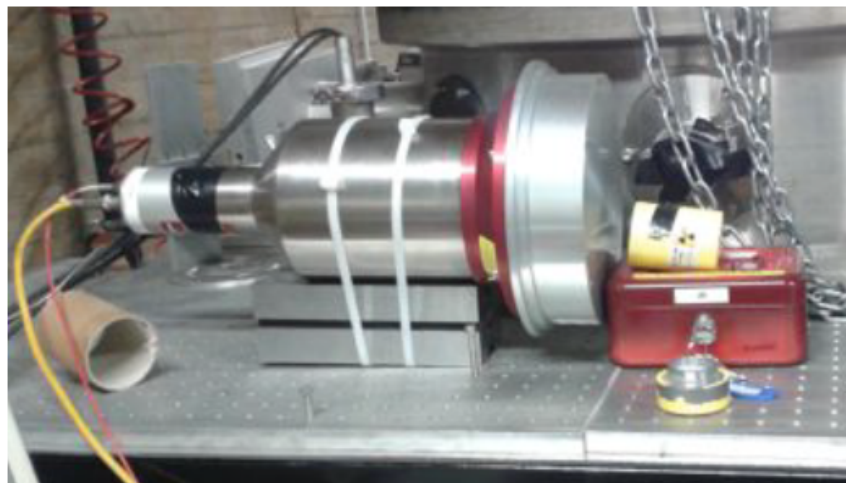


Figure 2. Scintillator EJ301 coupled with phototube.

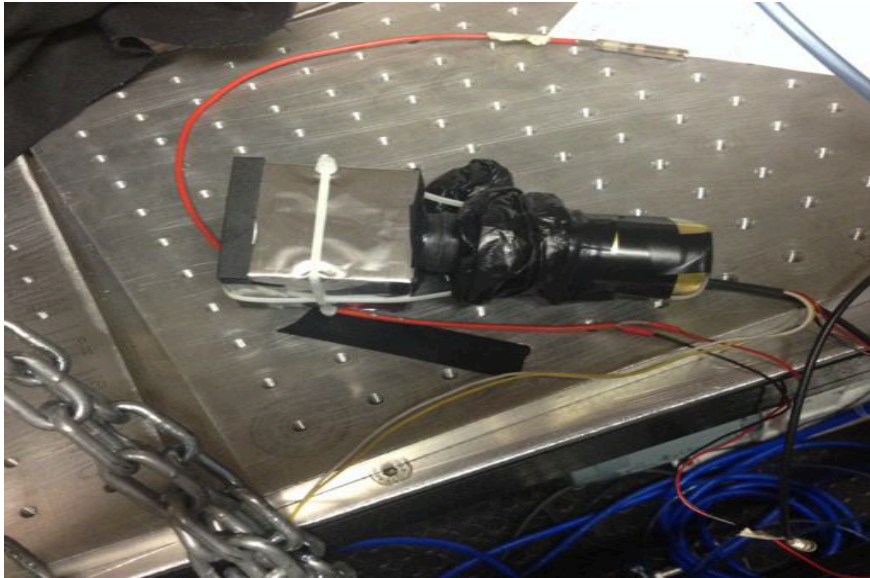


Figure 3. Scintillator EJ299 assembled with phototube.

The circuit, called BaF Pro [17] [18], is based on an analogic fast stretcher generating highly performing signals for PSD and timing purposes. A beam test has demonstrated a low detection threshold, a good pulse-shape discrimination even at low energies and a wide dynamic range for measurement of the neutrons energy. The voltage generated by the photon interaction of PMT, are send to BaF Pro.

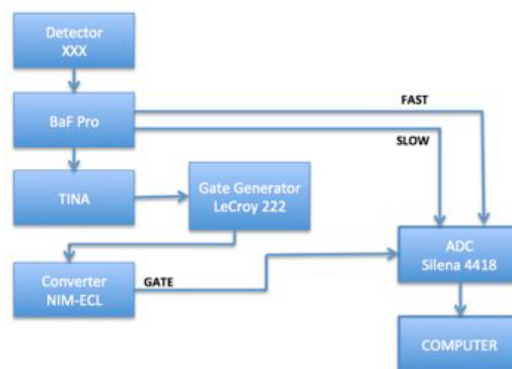


Figure 4. Block diagram of the electronic for the PSD.

The 16-channel BaF-pro module makes use of a sophisticated analog fast stretcher circuit to determine the fast component of the light output of the scintillator (hereafter indicated as “fast”) and an integration section that provides the total energy of the signal (hereafter indicated as “slow”).



Figure 5. BaF-Pro electronics.

Finally, a computer recorded the Fast and Slow components produced by the light collection system. Techniques for accurate discrimination between neutrons and photons interacting with scintillators have been established for a long time. The PSD techniques used to distinguish between the pulses from neutrons and the pulses from gamma rays rely on the differences in the pulse shapes produced. The goal of this research effort was to test the ability of a polyvinyltoluene research sample to produce recordable, distinguishable signals in response to gamma rays and neutrons. Pulse shape discrimination was performed to identify if the signal was generated by a gamma ray or a neutron. The results of such separation are shown in fig 6 and 7 for EJ301 and EJ299 respectively (neutrons are bounded in a red polygon).

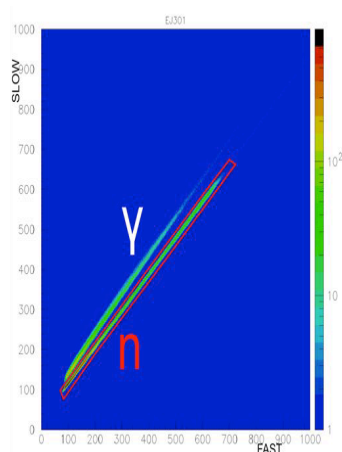


Figure 6. Pulse shape discrimination(PSD) performance for EJ301.

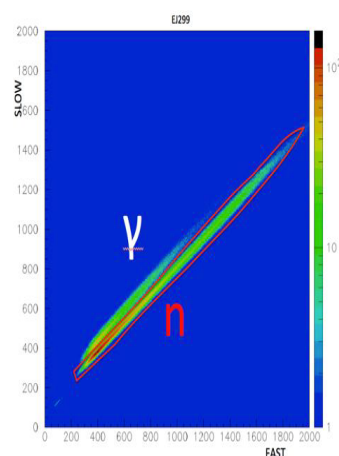


Figure 7. Pulse-shape discrimination(PSD) performance for EJ299.

Pulse shape analysis allowed the definition of a figure of merit as an indicative parameter for the neutron/gamma discrimination. Any detector with a Factor Of Merit (FOM) above 0.58, that is $FOM = \frac{S}{\delta_{neutrons} + \delta_{gammas}}$ where S is the separation between gamma and neutron peaks, and $\delta_{neutrons}$, δ_{gammas} are full width at half maximum (FWHM) of the corresponding peaks, can be considered to have

adequate PSD capability for fast neutron detection in the presence of gamma rays; both detectors exceed this merit factor.

Acknowledgment

This project has received funding from the European Union's Horizon 2020 research and innovation programme under grant agreement No 654002.

References

- [1] Cherubini S et al., 2004 *Eur Phys. J.A* Vol. 20 355-358
- [2] Musumarra A et al., 1996 *NIM A* 370 558-562
- [3] Amorini F et al., 1998 *Physical Review C* 58 987-995
- [4] Tudisco S et al., 2003 *Review of Scientific Instruments* 74 4485-4490
- [5] Lanzaò L et al., 2007 *European Biophysics Journal with biophysics letters* 336 823-829
- [6] Zaitseva N et al., 2012 *NIM. A* 668 88-93
- [7] Cappuzzello F et al., 2015 *Journal of Phys Conference Series* 630 012018
- [8] Negoita F et al., 2016 *Romanian Reports in Physics, Vol. 68, Supplement, P. S37–S144*
- [9] Cappuzzello F et al., 2016 *Eur.Phys.J.A* 52: 167
- [10] Cavallaro M et al., 2013 *NIM A* 700 65
- [11] Cavallaro M et al., 2016 *Phys. Rev. C* 93, 064323
- [12] Sciacca et al., 2006 *IEEE* 18 1633-1635
- [13] Mazzillo et al., 2007 *Sensors and actuators A* 138 306-312
- [14] Privitera S et al., 2008 *Sensors and actuators A* 8 4636-4655
- [15] Birks J B, 1964 *The Theory and Practice of Scintillation Counting, McMillan Co., New York*
- [16] Brooks F D, 1979 *NIM.* 162, 477
- [17] Boiano C et al., 2006 *IEEE Transactions on Nuclear Science* NS53(2) 444
- [18] Boiano C et al., 2008 *IEEE Nuclear Science Symposium Conference Record* N30-46